




Nebulizer Selection Flow Chart

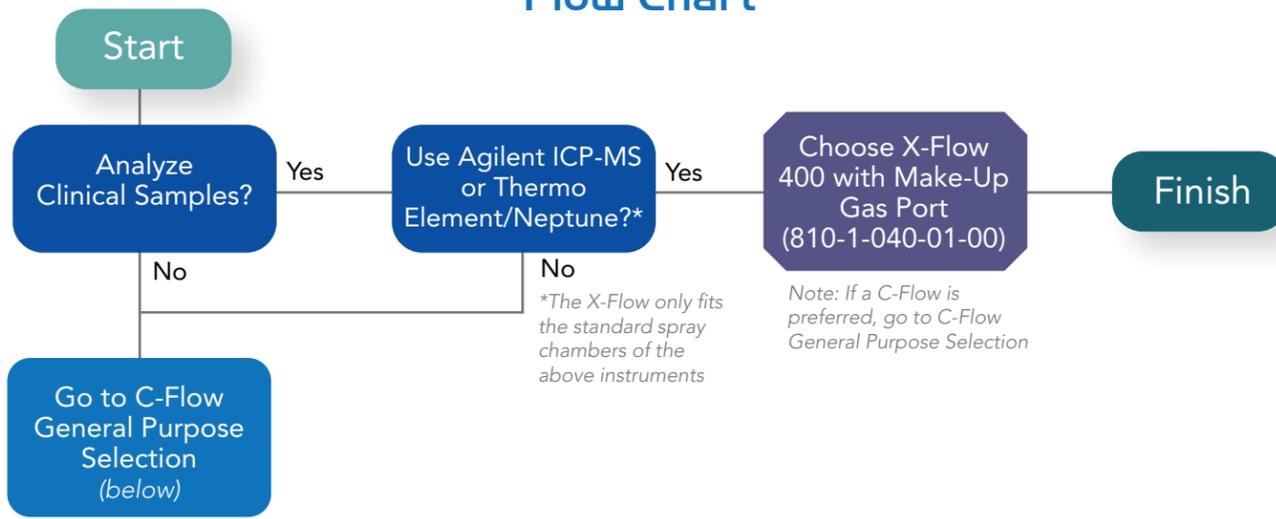

C-Flow (General Purpose) Selection Flow Chart

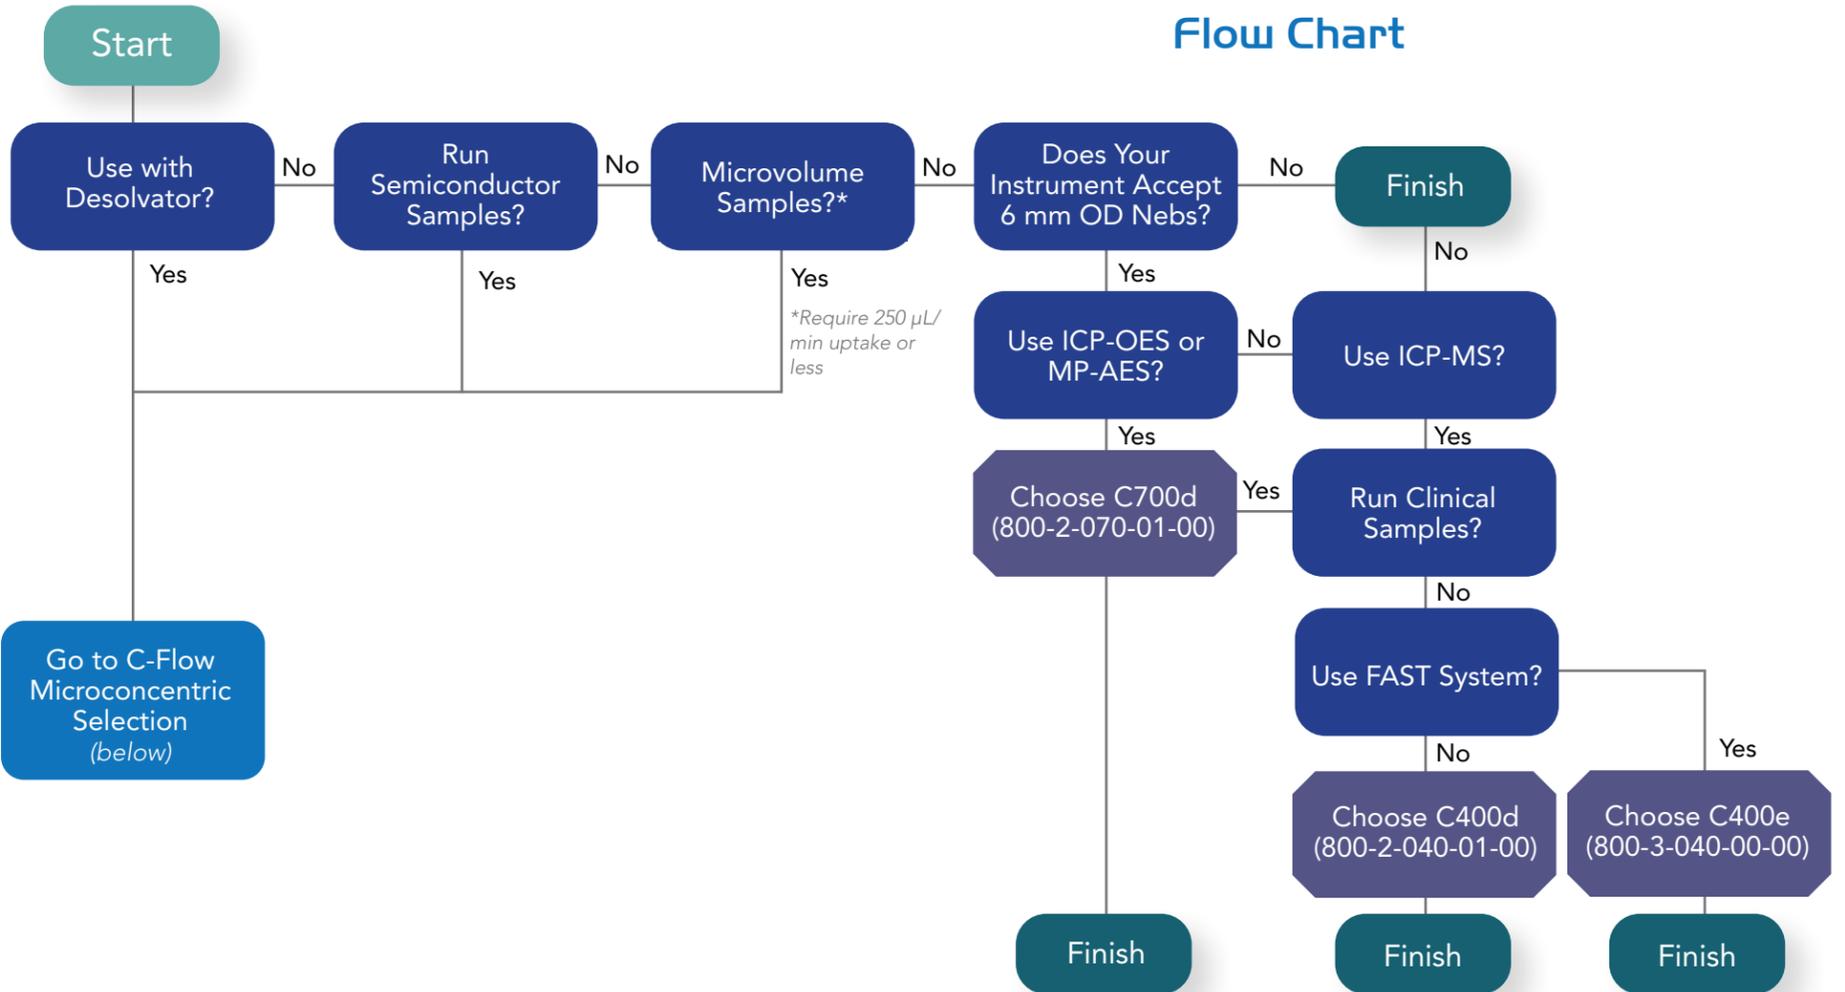

C-Flow (Microconcentric) Selection Flow Chart

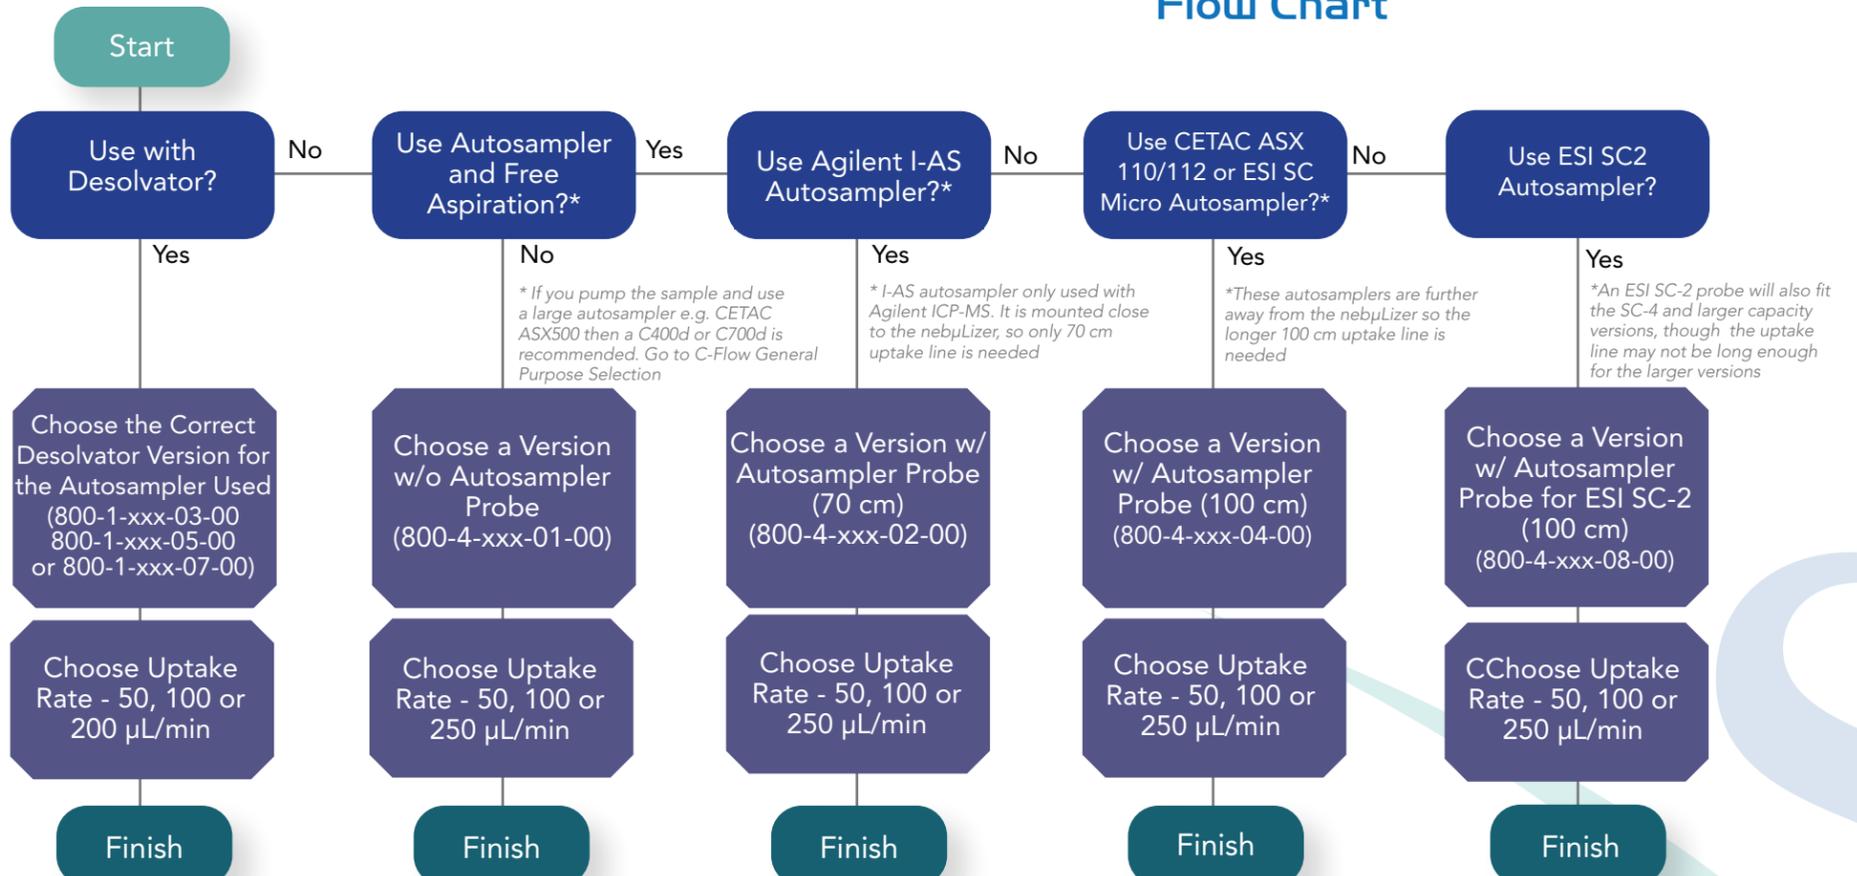

Note: Desolvator C-Flows are assembled at 110 °C. They can not be used for normal room temperature applications (i.e. non-desolvator)

Note: the carbon probe (100 cm) C-Flows have a slightly thicker probe to fit ESI autosamplers but can also be used with CETAC ASX 110/112